


## High level disinfection (HLD) is the industry standard to clean and reprocess conventional endoscopes.



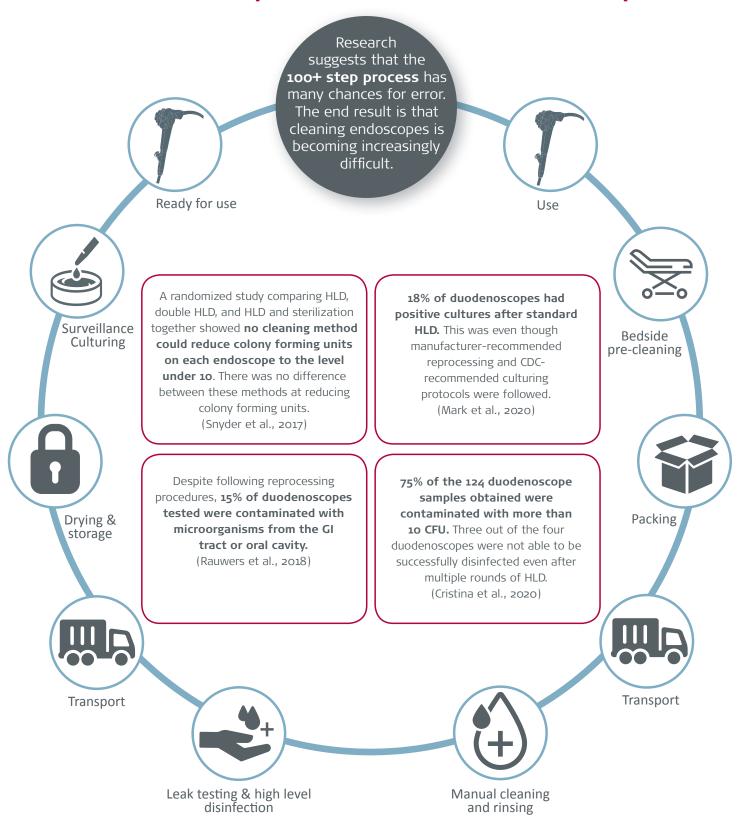

If you would like more information, or a customized analysis of the cost of reusable endoscopes in your facility, please contact our team of public health professionals at:

<u>us-healthecon@ambu.com</u>

## References:

Mark et al., Results of duodenoscope culture and quarantine after manufacturer-recommended cleaning process. Gastrointestinal Endoscopy. 2020 Jan 13, 91 (6): 1328-1333.

Cristina et al., Is Post-Reprocessing Microbiological Surveillance of Duodenoscopes Effective in Reducing the Potential Risk in Transmitting Pathogens?. Int J Environ Res Public Health. 2020 Jan; 17(1): 140.

Rauwers et al., High prevalence rate of digestive tract bacteria in duodenoscopes: a nationwide study. Gut. 2018 Sep;67(9):1637-1645

Snyder et al., Randomized Comparison of 3 High-Level Disinfection and Sterilization Procedures for Duodenoscopes. Gastroenterology. 2017 Oct;153(4):1018-1025

## Ambu Inc.

6230 Old Dobbin Lane Columbia, MD 21045 Tel. 800 262 8462 Fax 800 262 8673 ambuUSA.com